

MEASUREMENT PROTOCOL

No. PM_CT3_OPT_2015_03_03_21

Order number ZAK_Aremco_2014_01-3

Customer Aremco Products Inc.

Sample ID customer 840-MS
NTC 840_MS_01

Measured quantity spectral normal emissivity

Measurement method SNEHT

Temperature (T) 300°C

Polar angle (θ) 0°


Date 23.2.2015

Measured by Ing. Petra Honnerová, Ph.D.

Responsible person Ing. Jiri Martan, Ph.D.

tel.: +420 377 634 718

e-mail: jmartan@ntc.zcu.cz

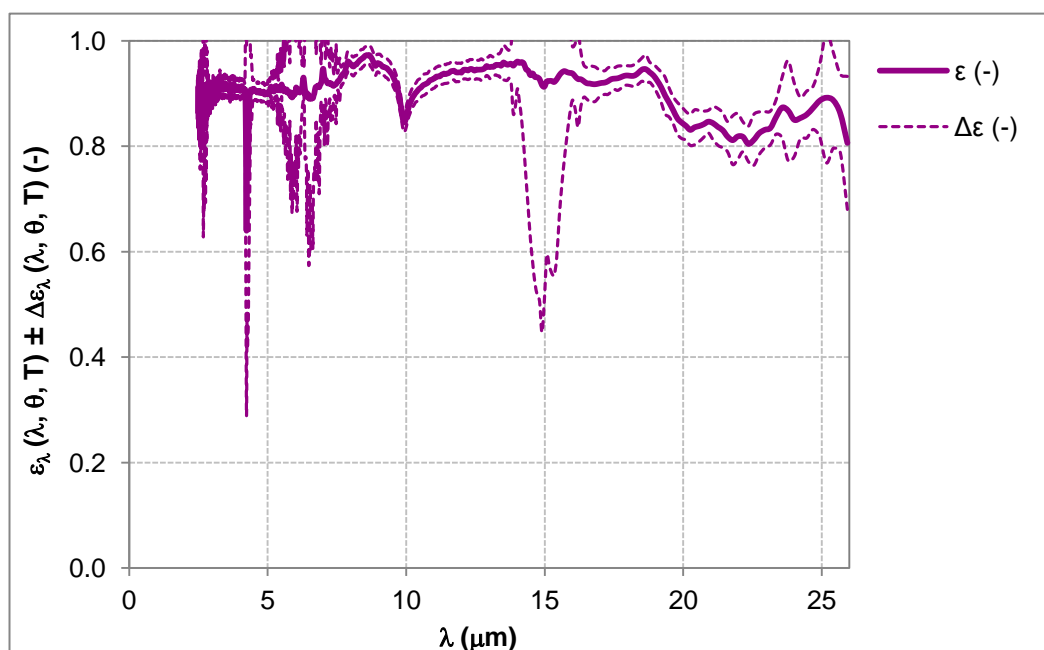

λ (μm)	2.5	3.5	4.7	8.3	10	12.5	17.5	20	25
$\varepsilon_{\lambda}(\lambda, \theta, T)$ (-)	0.852	0.913	0.902	0.962	0.858	0.946	0.928	0.845	0.887
$\Delta\varepsilon$ (-), $k = 2$	0.021	0.017	0.017	0.018	0.018	0.018	0.024	0.030	0.041